IPAD NFK200 Defibrillator

This is a new model of the iPAD series public access AED. The NFK200 is a simple to use, intuitive defibrillator allowing for quick and convenient pads access.





Matters

KEY FEATURES

- Easy access to pads from front panel
- Device and consumables status LED indicator
- CPR metronome, voice guidance, and graphic

INSTRUCTIONS

• Data transfer by USB


SAFETY

- Automatic internal discharge
- Daily / weekly / monthly self test
- Adult / paediatric mode change button

TECHNOLOGY

- Semi automated e cube biphasic defibrillation
- Combined adult / paediatric pads
- CPR step detection indicator for more effective CPR

NFK200 Defibrillator

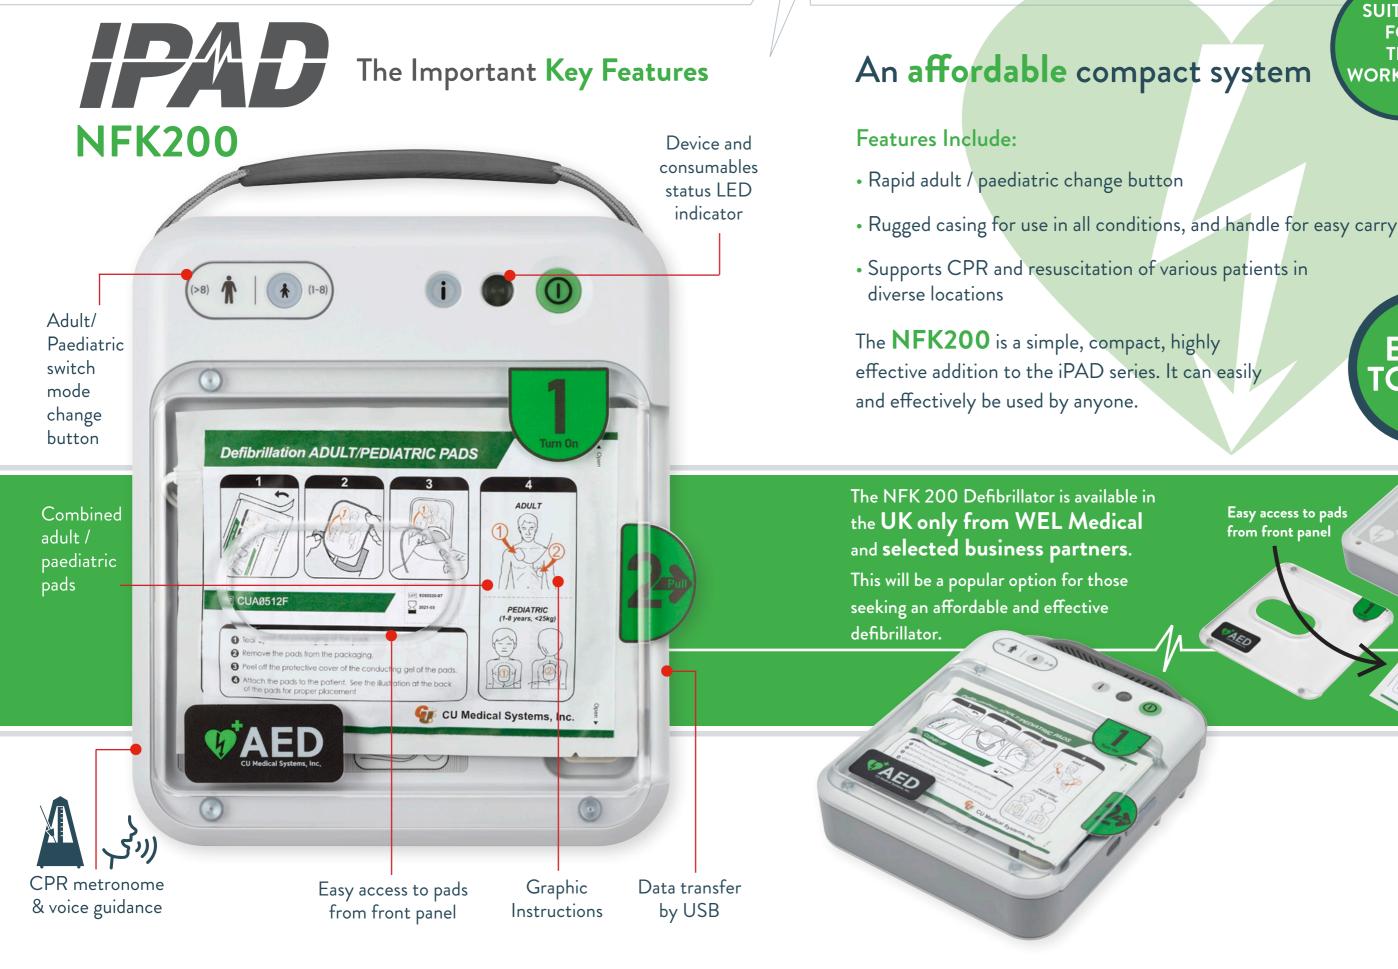



IPAD NFK200

Physical

· ·	
Dimensions	260mm x 220mm x 70mm (Width x Length x Height)
Weight	2.2kg (Including the battery pack and pads)
Environmental	
Operating Conditions	Temperature: 0°C ~ 50°C (32°F ~ 122°F) Humidity: 5 % to 95 % (non-condensing)
Storage Conditions	Temperature: 0°C ~ 50°C (32°F ~ 122°F) Humidity: 5 % to 95 % (non-condensing)
Transport Conditions	Temperature: -20°C ~ 60°C (-4°F ~ 140°F) Humidity: 5 % to 95 % (non-condensing)
Altitude	0 to 4,572 m (0 to 15,000 ft.)
Drop	Withstands 0.7 meter drop to any edge, corner or surface
Vibration	Operating: Meets MIL-STD-810G Fig.514.6E-1, Standby: Meets MIL-STD-810G Fig.514.6E-2
Sealing	IEC 60529:2013 IP42
ESD	Meets IEC 61000-4-2:2008
EMI (Radiated)	Meets IEC 60601-1-2 limits, method EN 55011: 2016+A1:2017, Group 1, Class B
EMI (Immunity)	Meets IEC 60601-1-2 limits, method EN 61000-4- 3:2006+A2:2010 Level 3 (10V/m 80MHz to 2.5GHz)

Defibrillator

Operating Mode	Semi-automated
Waveform	E-cube biphasic (Truncated exponential type)
Output Energy	150J at 50 Ω load for adults 50J at 50 Ω load for children
Charge Control	Controlled by an automated patient analysis system
Charging Time	Within 3 seconds from when the voice instruction, "An electric shock is needed" is issued.
Time from initiation of rhythm analysis	10 seconds with a new battery (even after the delivery of 15discharges at 150J) 12 seconds with a new battery (even after the delivery of 15 discharges at 200J)
Time from Power on to readiness for discharge	25 seconds with a new-fully charged battery (even after the delivery of 15 discharges at maximum energy)
Time from CPR to Shock	At least 6 seconds from the completion of CPR to shock delivery
Disarm	Patient's heart rhythm changes to non-shockable rhythm The SHOCK button is not pressed within 15 seconds

ECG Acquisition

Acquired ECG Lead	Lead II
Frequency Response	1 Hz to 30 Hz

ECG Analysis System

Impedance Range	25Ω to 175Ω
Shockable Rhythms	Ventricular Fibrillation or Fast Ventricular Tachycardia
Sensitivity and Specificity	Satisfies AAMI DF80

SPECIFICATIONS

Controls, Indicators, and Prompts

Controls	Power Button Shock Button Adult/Pediatric Selection Button
Indicators	Do-Not-Touch-Patient Pads Patch Position Indicators Status LED Indicator CPR Step and Detection Indicator Shock Button
Speaker	Provides voice prompts
Sound Level	75dB, 1m above speaker
Beeper	Provides various audible indications
Low Battery Indicator	Shown on the Status LED, announced via voice instruction

Self-Test

Automatic	Power On Self-Test, Run-time Self-Test Daily, Weekly, and Monthly Self-Test
Manual	Battery Pack Insertion Test

Battery Pack Long Life

Battery Type	12V DC, 4.2Ah LiMnO2, Disposable
Capacity	150 Joules - At least 200 Shocks for a new battery or 8 hours of operating time
Standby Life	At least 5 years from the date of manufacture
Temperature Ranges	Operating Temperature: 0°C ~ 50°C (32°F ~ 122°F) Storage Temperature: -20°C ~ 60°C (-4°F ~ 140°F)

Adult / Paediatric Defibrillation Pads

Surface Area	85cm²
Cable Length	120cm
Shelf Life	At least 36 months from the date of manufacture

Data Storage and Transfer

USB	External memory. Data may be copied from the internal memory to the USB.
File System	FAT32
Internal Memory Data Capacity	5 individual treatments, up to 3 hours per treatment

